

# UNCEMENTED THR AN OVERVIEW

Suresh Thomas  
Arthroplasty Fellow, Durham

# History

- Initial THRs uncemented
  - McKee / Farrar (1956-1960)
  - Hybrid cemented Thompson - uncemented cup




# Cont...

- Initial cemented THRs failing
  - ‘Cement disease’ - Charnley- Muller



# Cont...

- Ring type (late 1960's)
  - Metal on metal
  - Large femoral heads
  - Cup fixation with screw

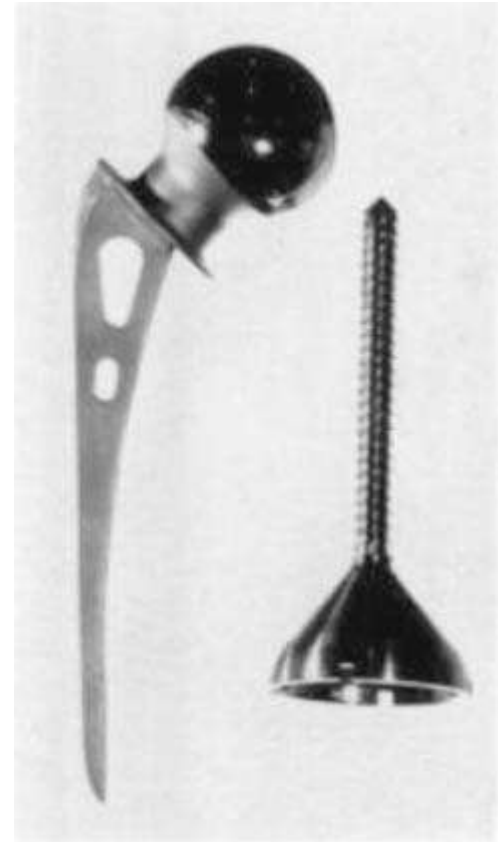

Cont...




# Cont...

- Smooth surface implants (1970's)
  - Strong adherence to bone not present
  - Locking of implant with window / fins
- Bony ingrowth
  - Pore size for maximum ingrowth
  - Pore size 100 to 200 $\mu\text{m}$

# Biologic Interdigitation

- Dynamic interface
- Bone remodelling
- Long lasting bond

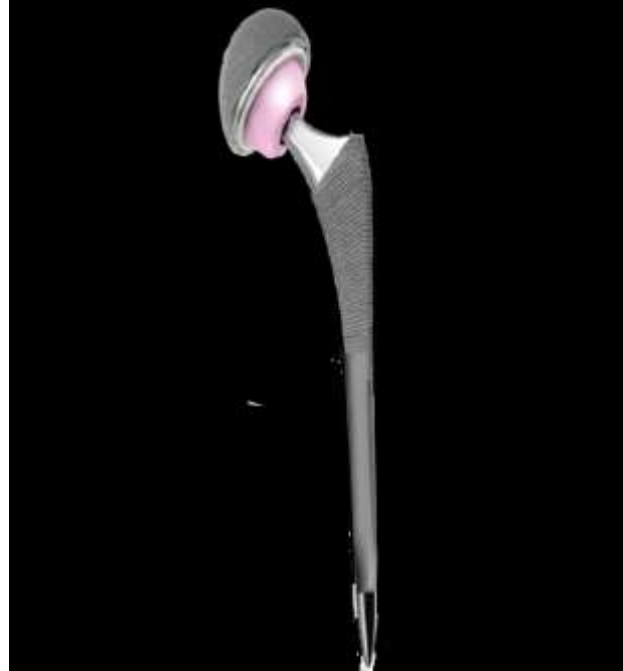

# Categories

- Porous coated metal surface
- Grit blast metal
- Hydroxyapatite

# Porous coated surface

- Allowing bony ingrowth
  - Proximal coating
    - Less stress shielding
  - Extensive coated stem
    - Stress shielding of proximal bone



# Optimal characteristics

- Pore size
  - 50 to 150 $\mu\text{m}$
- Porosity
  - 50%
- Optimal pore gaps
  - <50
- Acceptable micro motion
  - <150 $\mu\text{m}$

# Grit blasted metal

- Creates rough surface
  - Allowing bony ongrowth
- Surface roughness
  - Directly proportional to interface strength

# Hydroxyapatite

- Osteoconductive agent
  - Adjuvant to porous coated / grit blasted
  - More rapid closure of gaps
  - Shorter time to biological fixation




# Biological fixation techniques

- Rigid fixation (micro motion 50 to 150 $\mu$ m)
  - Press fit
    - Implant slightly larger than surrounding bone
    - Hoop stress around implant to reduce micromotion
  - Line to line
    - Bone size same as implant
    - Additional stabilisation (screws)
- Implant / bony contact
  - Cup/ femur implant size /contour




# Uncemented THR failures

Failures of cementless cup after operation

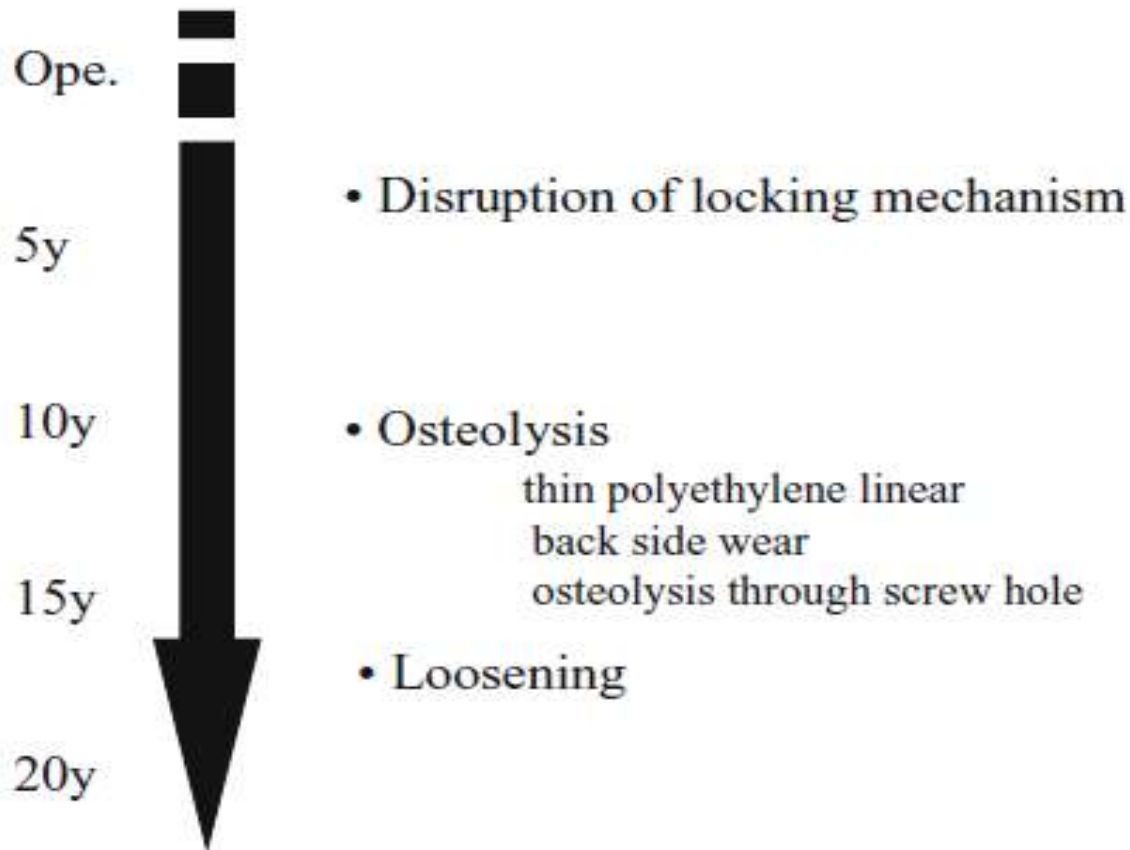

# Cont...

## Failures of cementless stem after operation

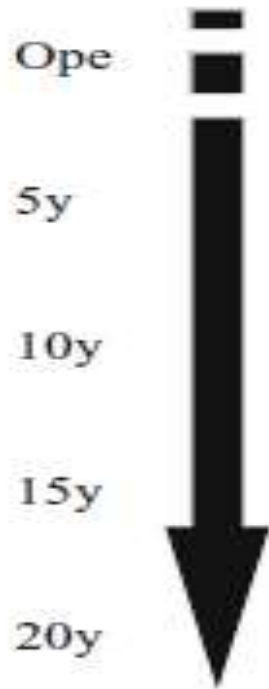

- Intra-operative fracture
- Stress shielding
- Fracture due to stress shielding
- Osteolysis
- Loosening



# Cont...

**Bone-ingrown**  
94.7%

**Stable fibrous**  
4%

**Unstable**  
1.3%



Cont...




# NJR data 2014

Fixation	Number (%)	Bearing surface within fixation group	Number (%)
All cases	620,400 (100.0%)		620,400 (100.0%)
All cemented	228,196 (36.8%)	MoP	201,246 (88.2%*)
		MoM	1,277 (0.6%)
		CoP	20,317 (8.9%)
		Others/unsure	5,356 (2.4%)
All uncemented	240,087 (38.7%)	MoP	88,994 (37.1%)
		MoM	28,658 (11.9%)
		CoP	34,619 (14.4%)
		CoC	81,205 (33.8%)
		CoM	2,074 (0.9%)
		Others/unsure	4,537 (1.9%)
All hybrid	100,940 (16.3%)	MoP	65,554 (64.9%)
		MoM	2,400 (2.4%)
		CoP	13,556 (13.4%)
		CoC	17,448 (17.3%)
		Others/unsure	1,982 (2.0%)
All reverse hybrid	14,675 (2.4%)	MoP	9,982 (68.0%)
		CoP	4,603 (31.4%)
		Others/unsure	90 (0.6%)
All resurfacing	36,462 (5.9%)	(MoM)	36,462 (100%)
Unsure	40 (<0.1%)	Unsure	40 (not applicable)

# Cont...

Figure 3.1


Temporal changes in percentages of each fixation method used in primary hip replacements.

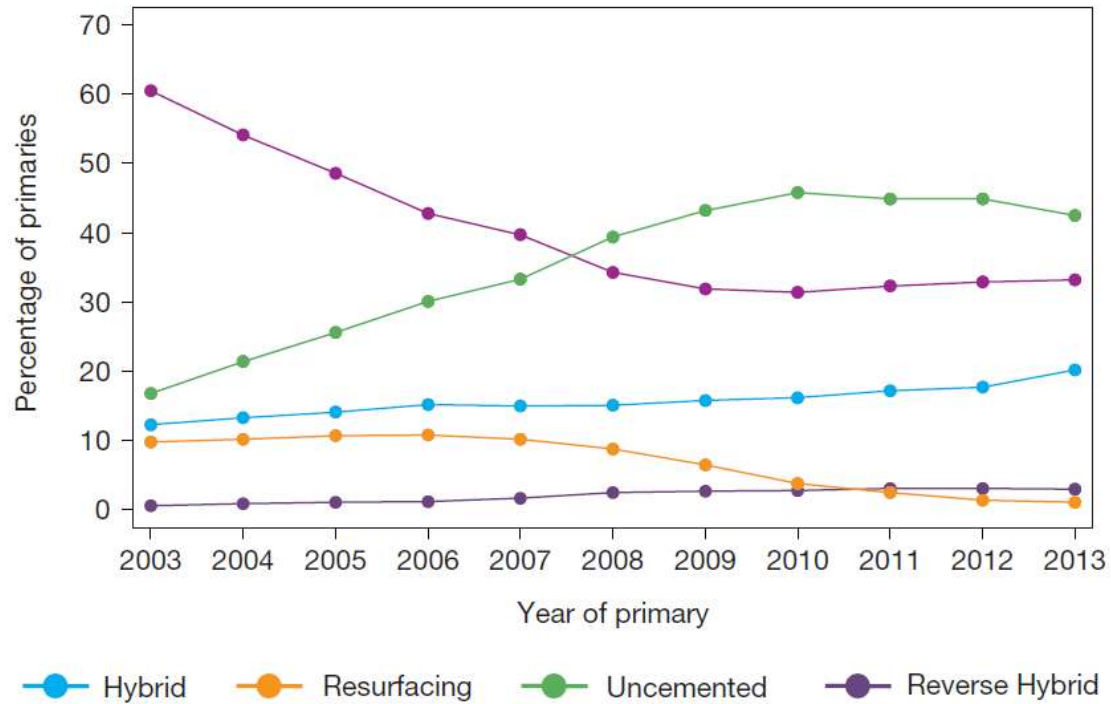

# Cont..

Figure 3.2 (b)

Temporal changes in percentages of each bearing surface used in **uncemented** primary hip replacements.

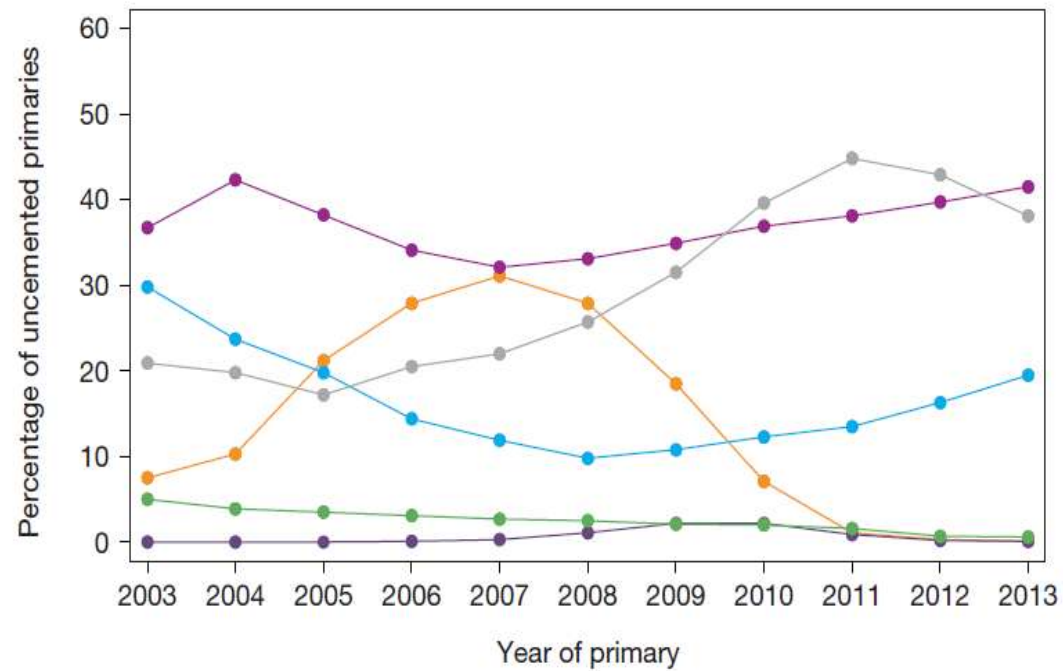

● Uncemented MoP ● Uncemented CoP ● Uncemented MoM ● Uncemented CoM

● Uncemented CoC ● Uncemented Other/Unsure

# Cont...

All uncemented	240,067	1.00 (0.96-1.04)	1.55 (1.50-1.60)	2.13 (2.07-2.20)	2.80 (2.72-2.88)	3.65 (3.55-3.75)	4.67 (4.54-4.80)	5.50 (5.35-5.65)	6.42 (6.22-6.62)	7.06 (6.81-7.31)	7.68 (7.34-8.03)
Uncemented by bearing surface:											
MoP	88,904	1.07 (1.00-1.14)	1.52 (1.43-1.60)	1.90 (1.80-2.00)	2.15 (2.04-2.26)	2.44 (2.31-2.57)	2.80 (2.66-2.95)	3.09 (2.90-3.27)	3.57 (3.34-3.81)	3.92 (3.64-4.23)	3.98 (3.67-4.31)
MoM	28,658	1.03 (0.92-1.16)	2.02 (1.88-2.19)	3.38 (3.18-3.60)	5.31 (5.05-5.58)	7.87 (7.35-8.00)	10.58 (10.18-11.00)	13.11 (12.61-13.64)	16.01 (15.31-16.73)	18.50 (17.47-19.59)	21.02 (19.81-24.22)
CoP	34,619	0.84 (0.74-0.94)	1.20 (1.08-1.33)	1.58 (1.44-1.74)	1.88 (1.72-2.06)	2.17 (1.99-2.38)	2.41 (2.20-2.64)	2.64 (2.40-2.90)	2.93 (2.65-3.24)	3.17 (2.84-3.54)	3.73 (3.22-4.33)
CoC	81,205	0.96 (0.89-1.03)	1.40 (1.40-1.58)	1.80 (1.79-2.00)	2.24 (2.12-2.36)	2.61 (2.46-2.78)	2.98 (2.81-3.17)	3.33 (3.11-3.56)	3.73 (3.45-4.04)	4.06 (3.70-4.46)	4.75 (4.11-5.47)
CoM	2,074	0.89 (0.40-1.14)	1.53 (1.08-2.18)	2.85 (2.19-3.70)	3.96 (3.12-5.02)	5.03 (3.87-6.51)	5.03 (3.87-6.51)	5.03 (3.87-6.51)	-	-	-
Others/unsure	4,537	1.25 (0.96-1.62)	1.74 (1.30-2.17)	2.24 (1.83-2.73)	2.70 (2.24-3.28)	3.22 (2.69-3.86)	3.93 (3.30-4.69)	4.39 (3.67-5.24)	5.20 (4.27-6.31)	6.11 (4.89-7.62)	6.11 (4.89-7.62)


# Cont...

Fixation/ bearing types	Age at primary (years)	Males					Females						
		n	Years from primary operation					n	Years from primary operation				
			1 year	3 years	5 years	7 years	10 years		1 year	3 years	5 years	7 years	10 years
All uncemented													
	<55	18,615	0.90 (0.77-1.05)	2.75 (2.49-3.04)	4.89 (4.47-5.33)	7.10 (6.49-7.75)	10.41 (9.04-11.96)	20,948	0.95 (0.83-1.10)	2.62 (2.38-2.88)	5.13 (4.74-5.57)	8.15 (7.53-8.83)	10.66 (9.62-11.81)
	55-64	32,236	0.92 (0.82-1.03)	2.26 (2.09-2.45)	3.96 (3.69-4.25)	6.11 (5.68-6.56)	8.15 (7.24-9.16)	39,357	0.88 (0.79-0.98)	2.11 (1.96-2.27)	3.98 (3.73-4.24)	6.18 (5.80-6.58)	8.96 (8.10-9.89)
	65-74	36,065	1.03 (0.93-1.14)	2.05 (1.89-2.22)	3.16 (2.94-3.40)	4.64 (4.30-5.02)	6.39 (5.72-7.13)	47,134	0.91 (0.83-1.00)	1.82 (1.69-1.96)	3.22 (3.01-3.44)	4.97 (4.65-5.33)	6.86 (6.21-7.58)
	75+	17,628	1.26 (1.10-1.44)	2.04 (1.82-2.29)	2.82 (2.52-3.16)	3.36 (2.95-3.82)	4.30 (3.51-5.41)	27,987	1.27 (1.14-1.41)	1.88 (1.72-2.00)	2.56 (2.34-2.81)	3.38 (3.05-3.75)	4.58 (3.68-5.72)

# Cont...

**Figure 3.5**

Comparison of cumulative probability of revision (Kaplan-Meier estimates) for **uncemented** hips with different bearing surfaces.

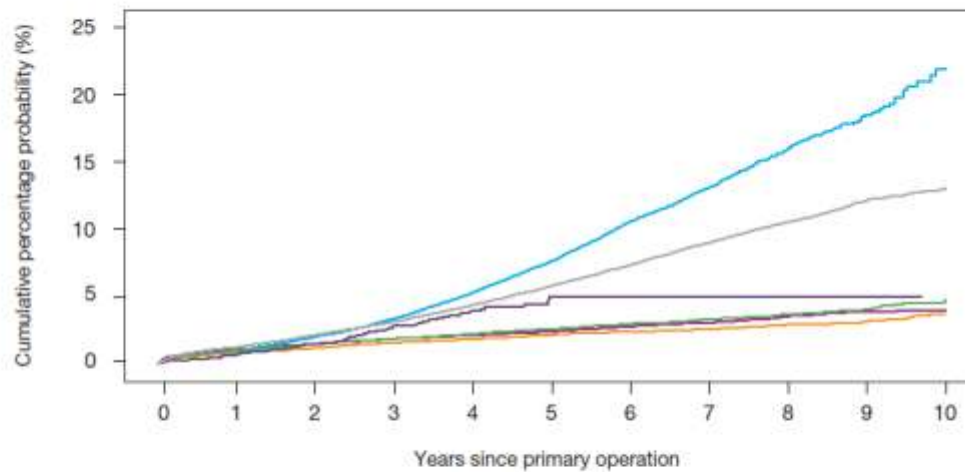

Numbers at risk

— Uncemented MoP	66,994	73,559	58,934	45,872	33,890	23,938	15,803	9,971	5,763	2,578	644
— Uncemented MoM	28,658	28,030	27,389	26,323	23,367	17,793	11,034	5,837	2,342	624	131
— Uncemented CoP	34,619	27,801	21,960	17,380	13,346	10,200	7,681	5,401	3,508	1,770	586
— Uncemented CoC	81,205	67,690	52,636	37,920	25,412	16,466	10,013	5,821	3,090	1,492	431
— Uncemented CoM	2,074	2,017	1,932	1,600	910	316	58	12	2	1	0
— Resurfacing	36,462	35,092	33,638	31,417	28,370	23,819	18,093	12,235	7,573	3,773	1,250

# Summary

- Concept of biological fixation
  - Optimal surface property
  - Optimal micro movement
  - Optimal pore size
  - Optimal fixation
  - Optimal implant size / contour



Thank you